DRG No A0-204/78053 SHT 10 OF 16

DRAWING PRACTICE TO BS308 – THIRD ANGLE PROJECTION

LAKESHORE 625 PSU 5V, 60A UNIT 1

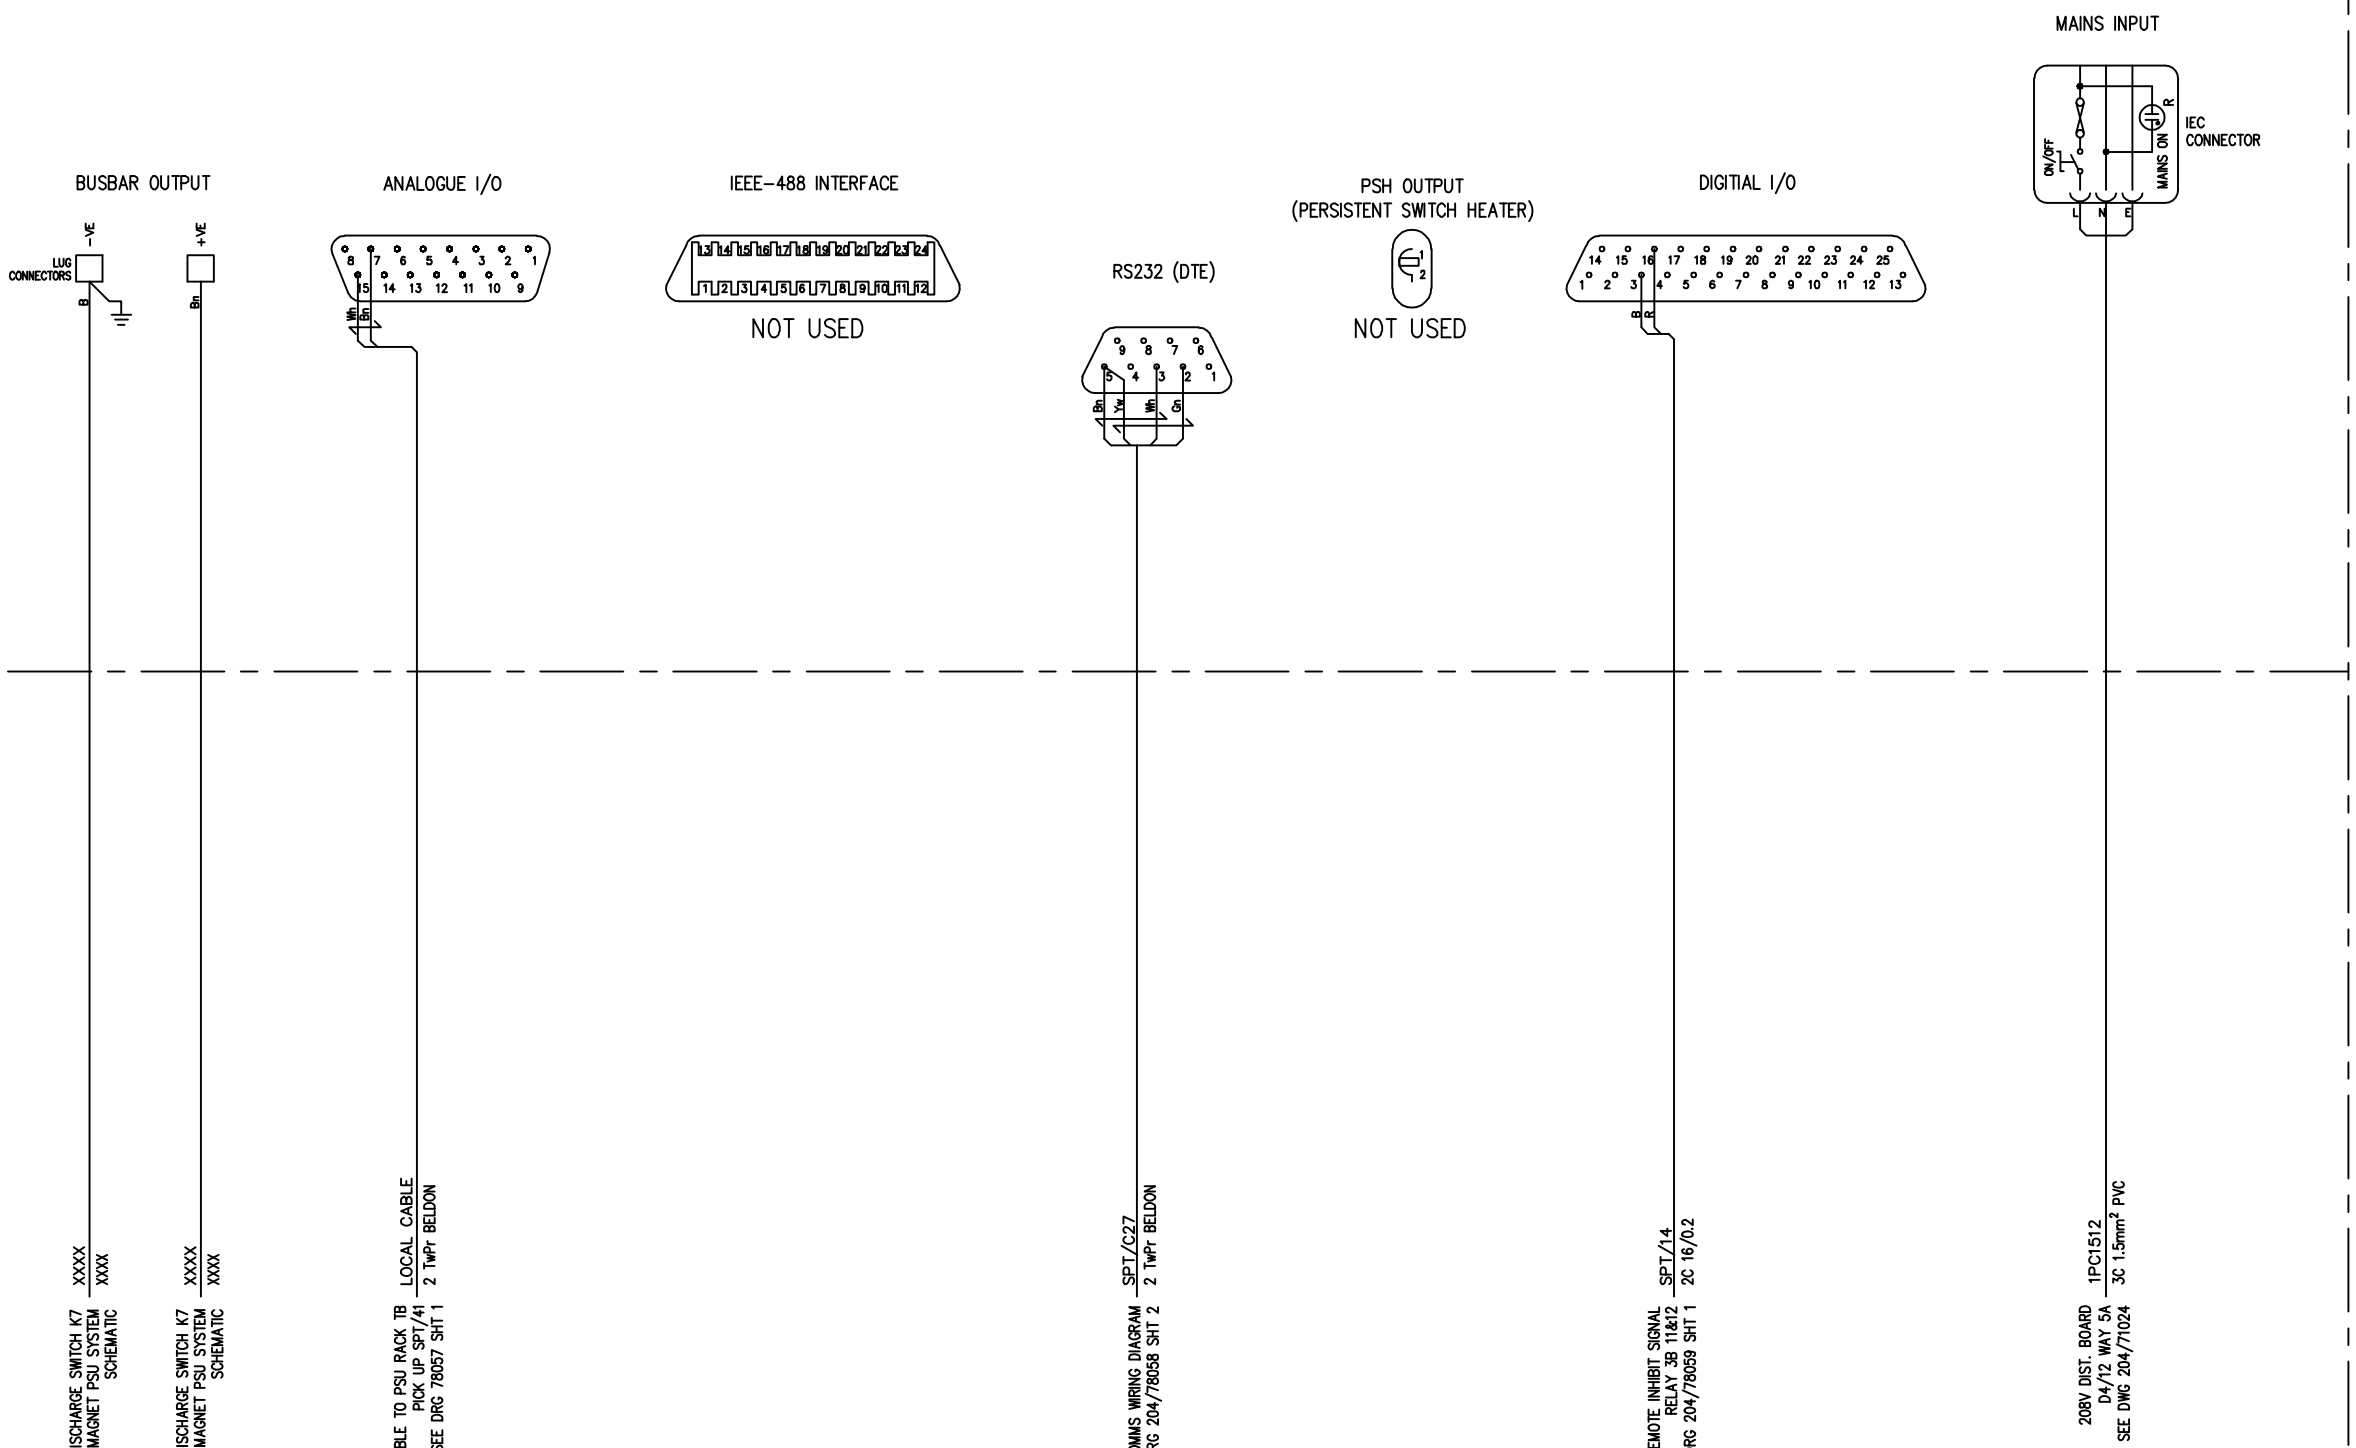

RS232 (DTE)



9W (M)
D-TYPE

ANALOGUE I/O

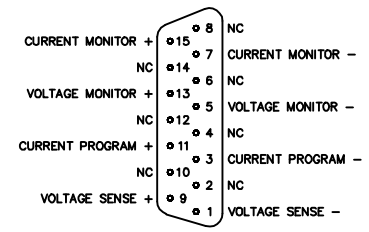

9W (M)
D-TYPE

DIGITIAL I/O

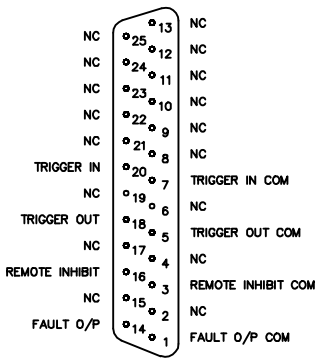

IEEE-488 INTERFACE

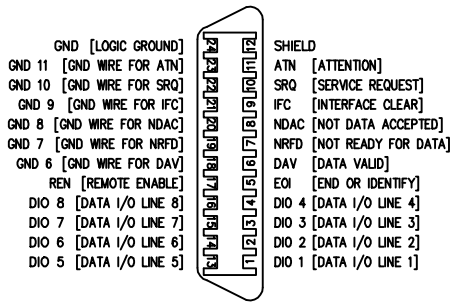

KEY

NC – NOT CONNECTED

NOTES

1) UNUSED CORES TO BE SLEEVED OFF AND TIED BACK

REF DRAWINGS

204/78050 SPECTROMETER TEST RACK BLOCK DIAGRAM
204/78055 SPECTROMETER TEST RACK CANBUS/VME NETWORK
204/78057 PSU/COMMS/SIGNAL CONVERTER WIRING DIAGRAM
204/78059 SPECTROMETER TEST RACK CANBUS WIRING DIAGRAM
204/78052 SPECTROMETER TEST RACK POWER DIST DIAGRAM
204/78056 SPECTROMETER TEST RACK DAC/ADC WIRING DIAGRAM
204/78058 SPECTROMETER TEST RACK RS232 WIRING DIAGRAM

A FIRST ISSUE

SCALE 0

ALL DIMENTIONS IN MILLIMETERS UNLESS OTHERWISE STATED

DRN	P.A.D.	SCIENCE AND TECHNOLOGY FACILITIES COUNCIL DARESBURY LABORATORY CHESHIRE
DATE	15/10/11	
CKD	I.M.	TITLE MICE COOLING CHANNEL TEST RACK EQUIPMENT WIRING DIAGRAM
DATE	27/03/12	
CERT		
DATE		
APPD	I.M.	DRG No A0-204/78053 SHT 10 OF 16 ISSUE A
DATE	27/03/12	CAD PART No 204/78053-10

DRAWING LIST:– DL 204/78000

CONTRACTORS COMPANY
CONTRACTORS DRG No

ORIGINAL FRAME SIZE 1140mm X 790mm