DRG No A0-204/78053 SHT 8 OF 16

DRAWING PRACTICE TO BS308 – THIRD ANGLE PROJECTION

OMEGA DP 41-E

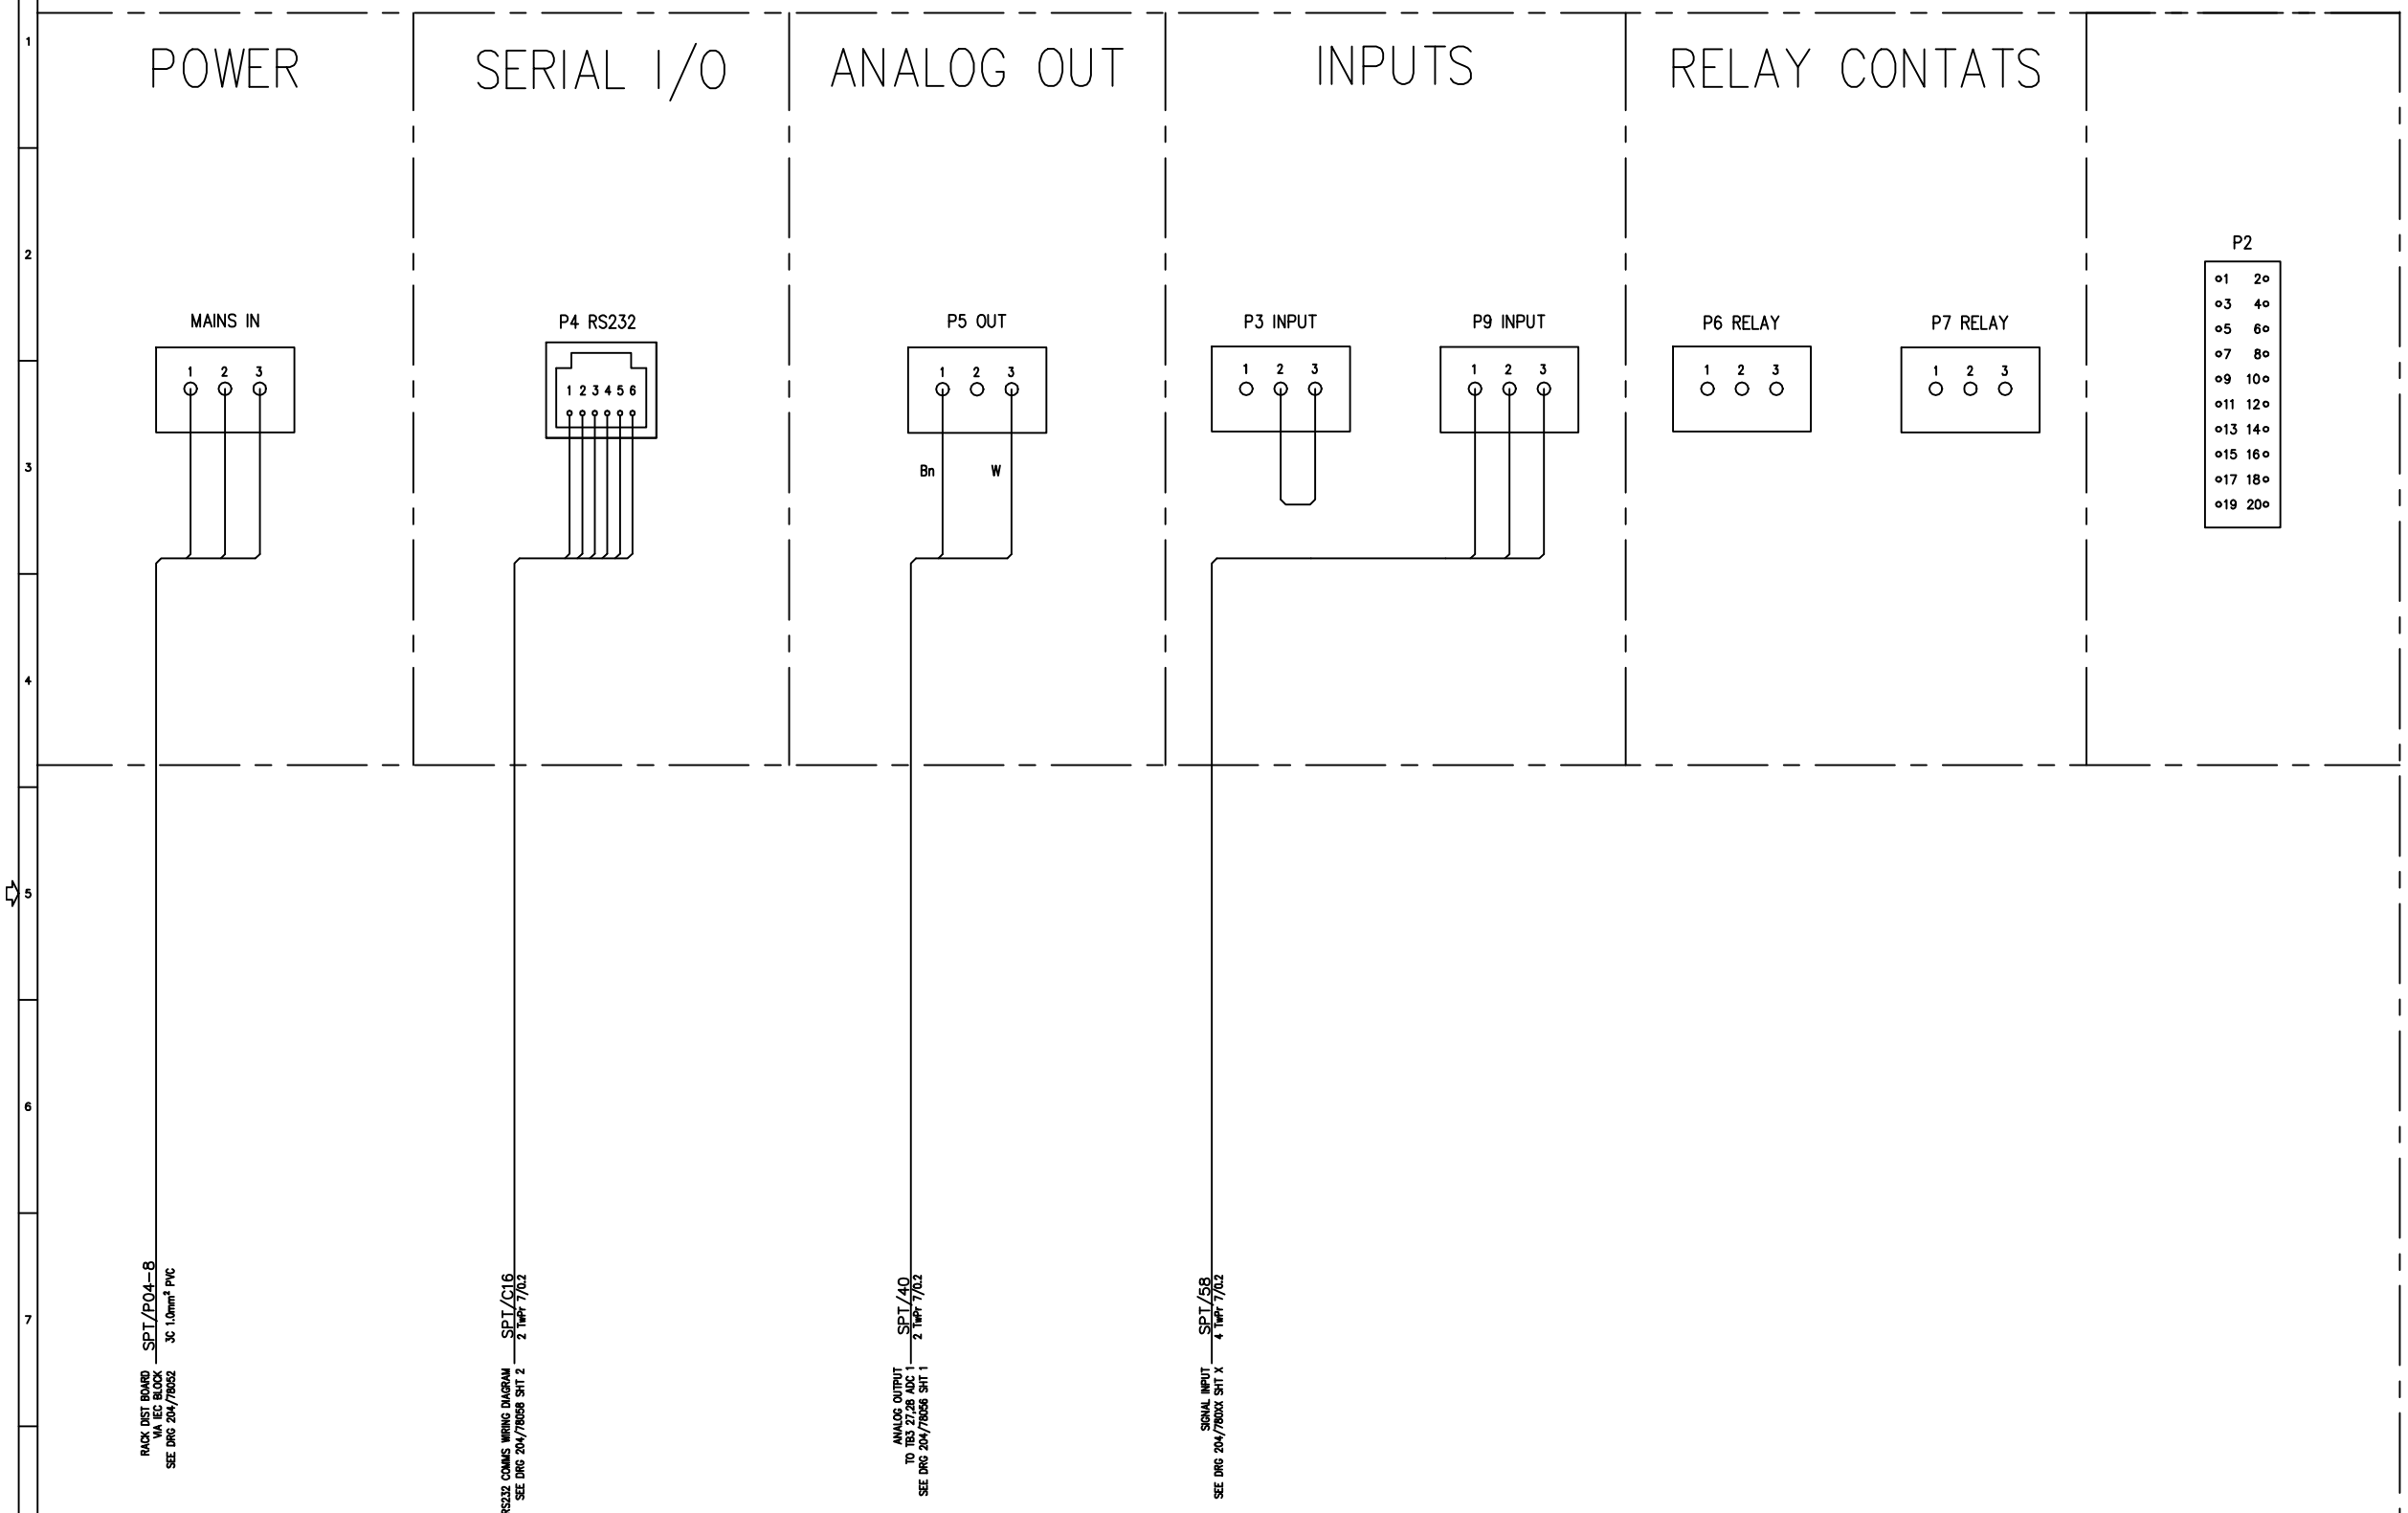

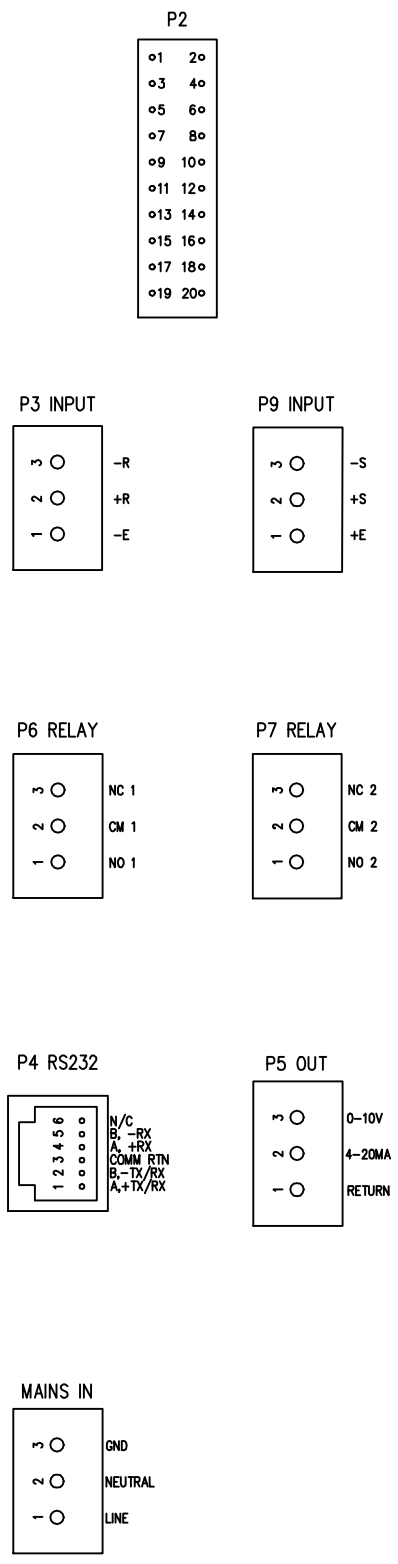

NOTES

1) UNUSED CORES TO BE SLEEVED OFF AND TIED BACK

REF DRAWINGS

204/78050 SPECTROMETER TEST RACK BLOCK DIAGRAM
204/78055 SPECTROMETER TEST RACK CANBUS/VME NETWORK
204/78057 PSU/COMMS/SIGNAL CONVERTER WIRING DIAGRAM
204/78059 SPECTROMETER TEST RACK CANBUS WIRING DIAGRAM
204/78052 SPECTROMETER TEST RACK POWER DIST DIAGRAM
204/78056 SPECTROMETER TEST RACK DAC/ADC WIRING DIAGRAM
204/78058 SPECTROMETER TEST RACK RS232 WIRING DIAGRAM

A	FIRST ISSUE	

SCALE 0

ALL DIMENTIONS IN MILLIMETERS UNLESS OTHERWISE STATED

DRN DATE	P.A.D. 15/10/11	SCIENCE AND TECHNOLOGY FACILITIES COUNCIL DARESBURY LABORATORY CHESHIRE
CKD DATE	I.M. 27/03/12	TITLE MICE COOLING CHANNEL TEST RACK EQUIPMENT WIRING DIAGRAM
CERT DATE		DRG No A0-204/78053 SHT 8 OF 16
APPD DATE	I.M. 27/03/12	CAD PART No 204/78053-8 ISSUE A

DRAWING LIST:- DL 204/78000

CONTRACTORS COMPANY
CONTRACTORS DRG No

ORIGINAL FRAME SIZE 1140mm X 790mm