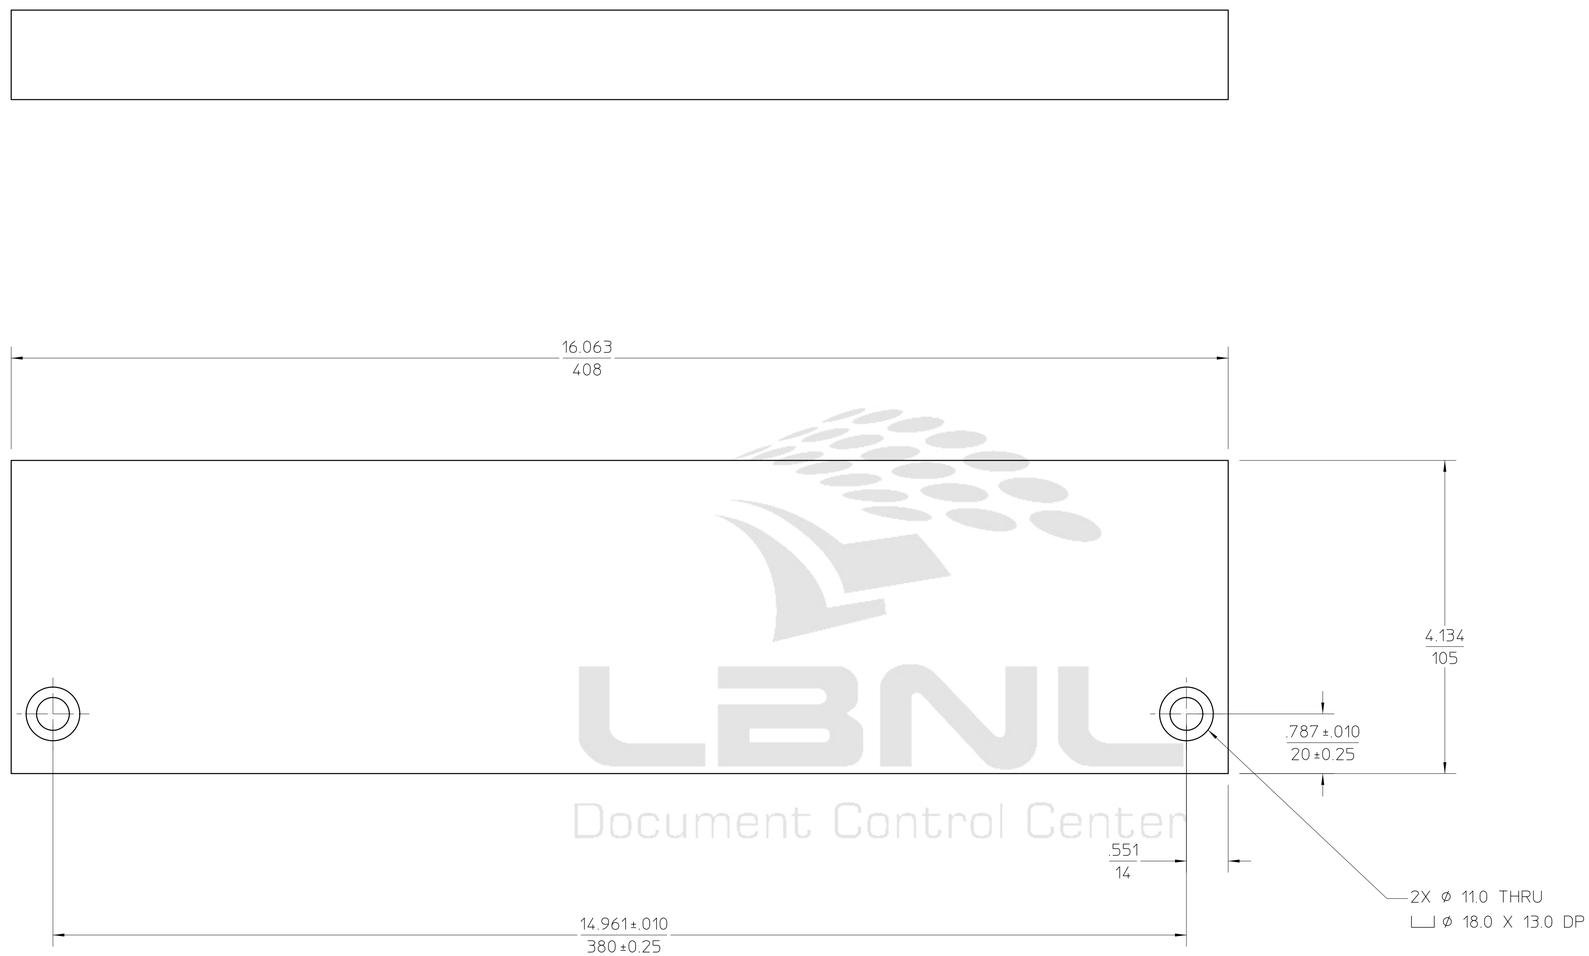

LBNL
Document Control Center

(UNIQUE ID NO.:AL-0008-9559)

NOTES,UNLESS OTHERWISE SPECIFIED:

1. THIS IS A ULTRA HIGH VACUUM COMPONENT AND REQUIRES SPECIAL ATTENTION TO AVOID CONTAMINATION. REFER TO LBNL ENGINEERING SPECIFICATION #M20013. HIGH VACUUM USE CLEANING.

2. TOLERANCES SHOWN IN TITLE BLOCK ARE IN INCHES.

REV	AUTHOR	APPROVER	DATE	CHANGE DESCRIPTION
A	rawlins	plate	07-26-20	INITIAL REVISION

UNLESS OTHERWISE SPECIFIED
TOLERANCES: X± .06 X.X± .03 X.XX± .020
FRACTIONS: ±1/64
ANGLES: ± 2°
MACH. SURFS.: 63 ✓ OR BETTER
REF:ASME Y14.5M-1994, THREADS ARE CLASS 2
BREAK EDGES .016 MAX. ON MACHINED WORK
REMOVE BURRS, WELD SPLATTER & LOOSE SCALE

MAT 2: . NOTES:
MAT 1: OFHC COPPER NOTES:

PROJECT NAME: Advanced Light Source
UNIQUE NUMBER: AL-0008-9559
DO NOT SCALE PRINT SCALE: 1 : 2
CATEGORY CODE: AL 4160
THIRD ANGLE PROJECTION

ERNEST ORLANDO LAWRENCE
BERKELEY NATIONAL LABORATORY
UNIVERSITY OF CALIFORNIA
ALS - INSERTION DEVICE BEAMLINES
BL 6.0 FRONT END
OUTER ABSORBER 2 LH

SHEET 1 OF 1 SIZE: D DWG NO: 26B595 REV A

AUTO GENERATED PDF
Jul 27 2004 13:57:56 PDT

Officially Released to the LBNL Document Control Center
Released: July 26th, 2004 DCC Auth Key: WT3652CHO
Downloaded by: Daniel Pulsifer at December 01, 2004 14:27:03