

8

7

6

5

4





3

1

DWG. NO.		SIZE	REV.	SH.	
2515534		A	1		
2	-	1	TUBE, PER ASTM A269		SS 304L
1	-	1	COLLAR		SS 304L
ITEM	PART NO	REQD	DESCRIPTION		MATERIAL

NOTES: (UNLESS OTHERWISE SPECIFIED)

- THIS IS A CRYOGENIC VACUUM COMPONENT.
- WELDING PROCEDURE: PER VENDOR SPECIFICATION WITH LBNL APPROVAL.
- CLEANING PROCEDURE : PER VENDOR SPECIFICATION WITH LBNL APPROVAL.
- PACKAGING AND STORAGE PROCEDURE OF THE COMPONENTS: PER VENDOR SPECIFICATION WITH LBNL APPROVAL.
- DIMENSIONS AND TOLERANCING PER ANSI Y14.5M-1982. UNITS ARE IN INCHES [mm] UNLESS OTHERWISE SPECIFIED.
- USE OF SULFUR OR SILICONE BEARING OILS, LUBRICANTS, OR COOLANTS ARE STRICTLY PROHIBITED.
- USE OF RESIN OR RUBBER BONDED ABRASIVES UNDER POWER IS STRICTLY PROHIBITED. USE VITREOUS BONDED ABRASIVES ONLY.
- VENDOR SUGGESTED CHANGES TO WELD PREPS; SUBJECT TO LBNL APPROVAL.
- FITTINGS MAY BE USED IN PLACE OF BENDS; SUBJECT TO LBNL APPROVAL.
- VENDOR SUGGESTED CHANGES TO TOLERANCES TO FACILITATE FABRICATION OR ASSEMBLY; SUBJECT TO LBNL APPROVAL.
- REMOVE ALL THE BURRS AND REAM THE ENDS FOR CIRCULARITY AND CLEAN ENDS.
- TUBE END SURFACE MUST BE PERPENDICULAR TO THE TUBE AXIS WITHIN +/- .010.
- PERFORM ACCEPTANCE TESTS PER SECTION 3.2 OF LBNL SPECIFICATION M856.
- A MARK DESIGNATING THE INSTALLED LENGTH WILL BE UTILIZED DURING FINAL INSTALLATION OF THE FEEDBOX ASSEMBLY. MARK, SCRIBE OR ETCH THIS LOCATION IN A PERMANENT MANNER, SUBJECT TO LBNL APPROVAL, TO AN ACCURACY OF ±0.063".
- PROVIDE A MINIMUM LENGTH OF 4.0" OF STRAIGHT, SMOOTH PIPE ON THE INDICATED SIDE OF THE INSTALLED LENGTH MARK FOR PIPE WELDING DURING FINAL INSTALLATION OF THE FEEDBOX ASSEMBLY.
- PIPE MUST BE STRAIGHT AND SMOOTH (NO BUMPS) FOR 0.5" ON EITHER SIDE OF THE CENTER-PLANE OF THE SUPPORT.
- CAP BOTH ENDS OF PIPE AFTER ACCEPTANCE TESTS PER SECTION 3.2 OF LBNL SPECIFICATION M856.

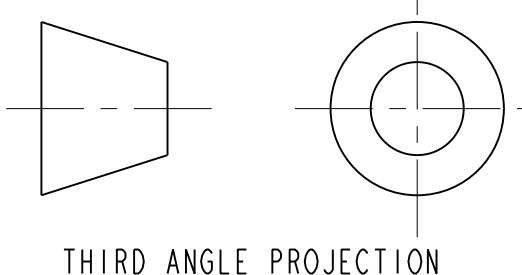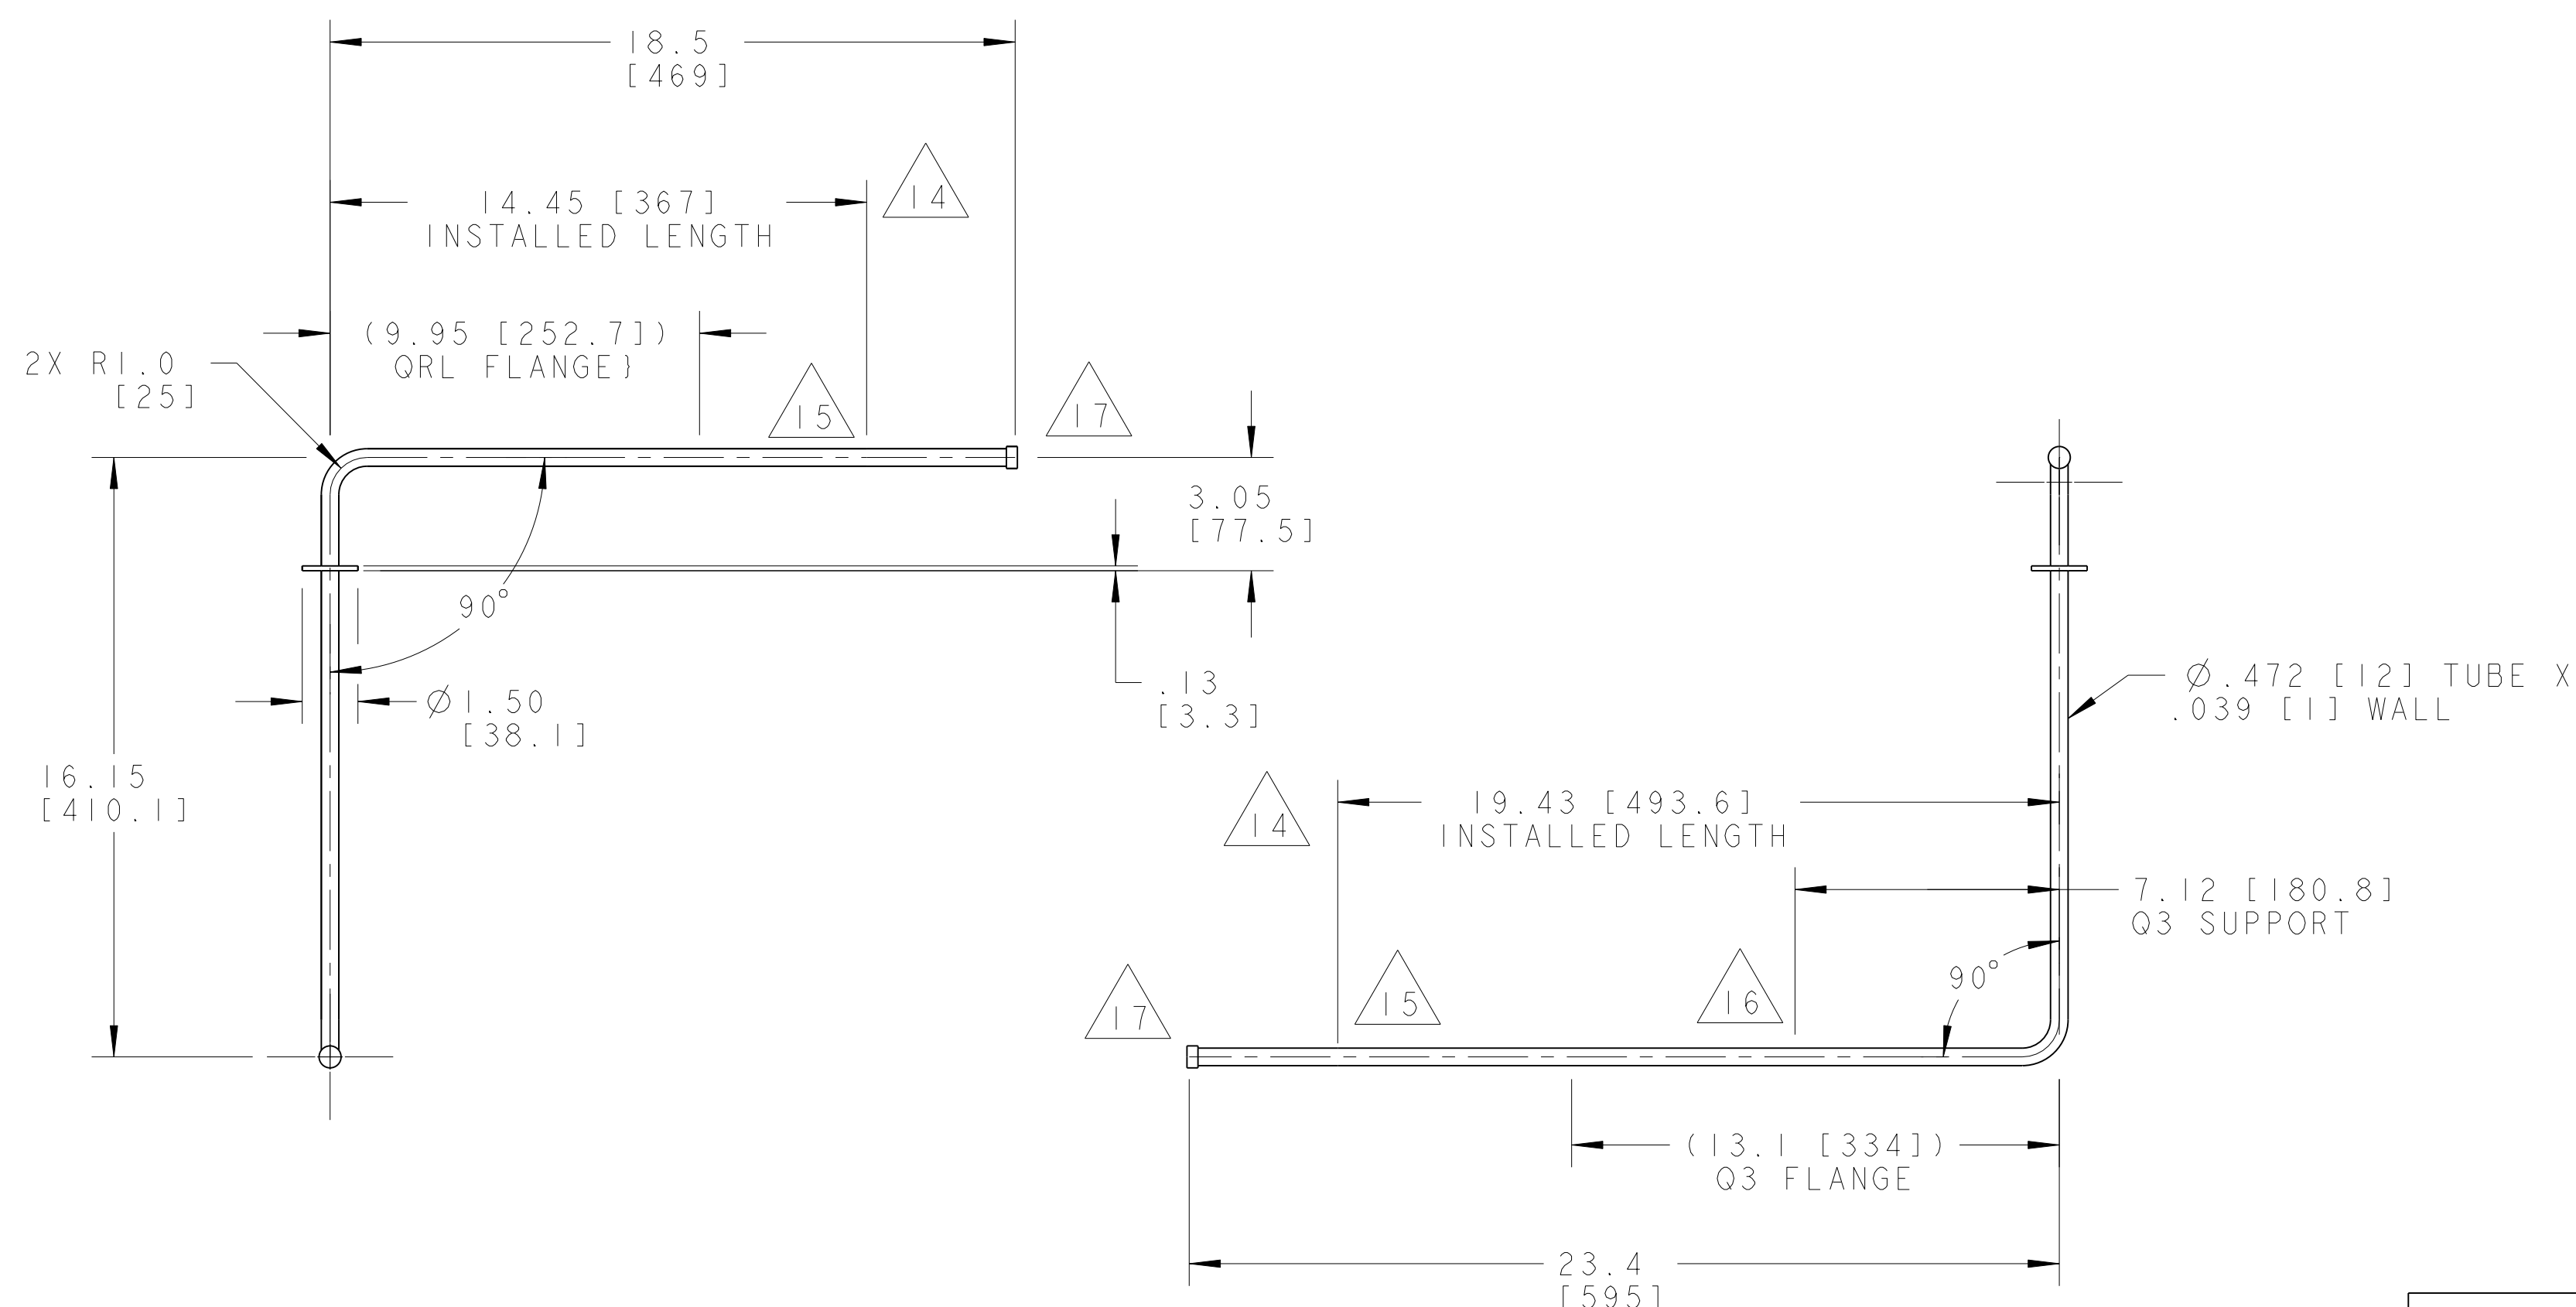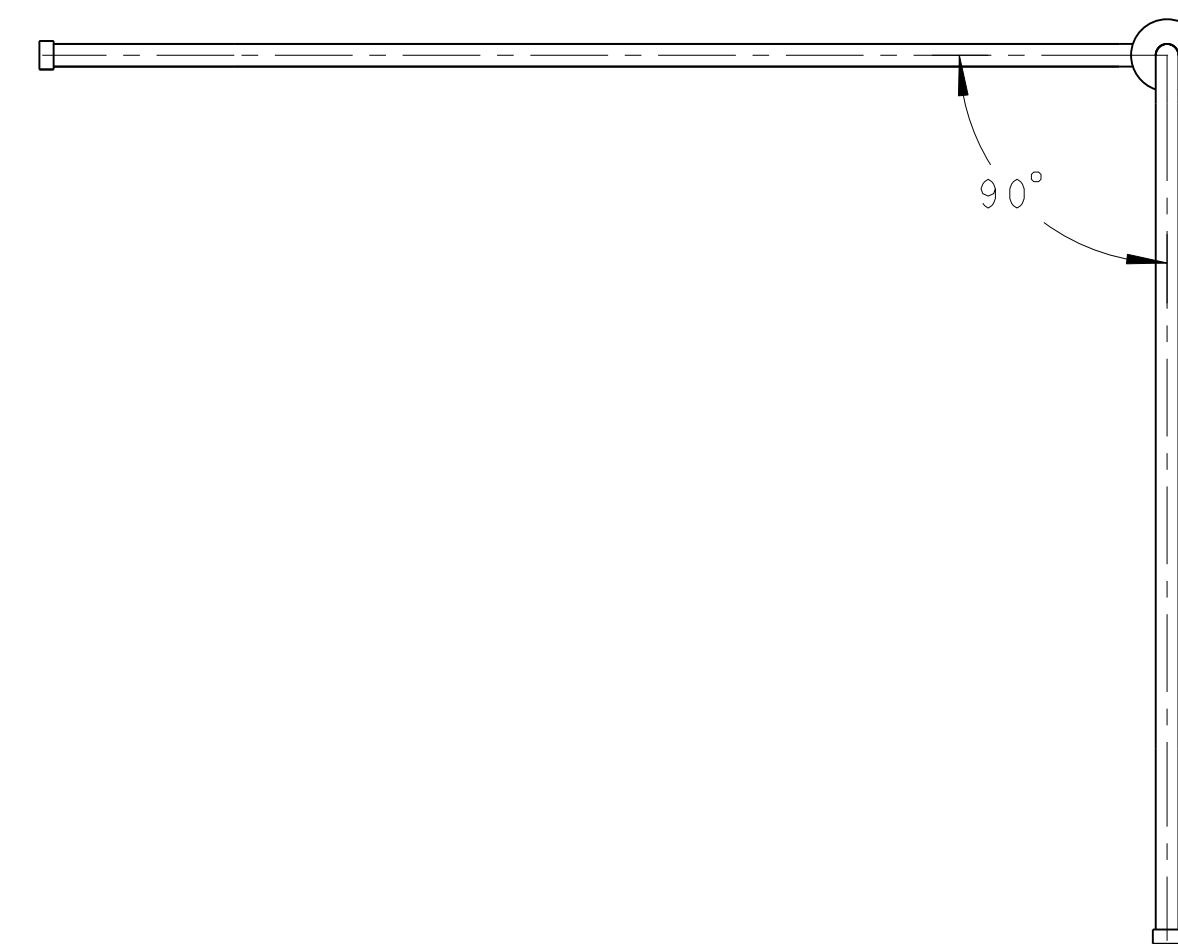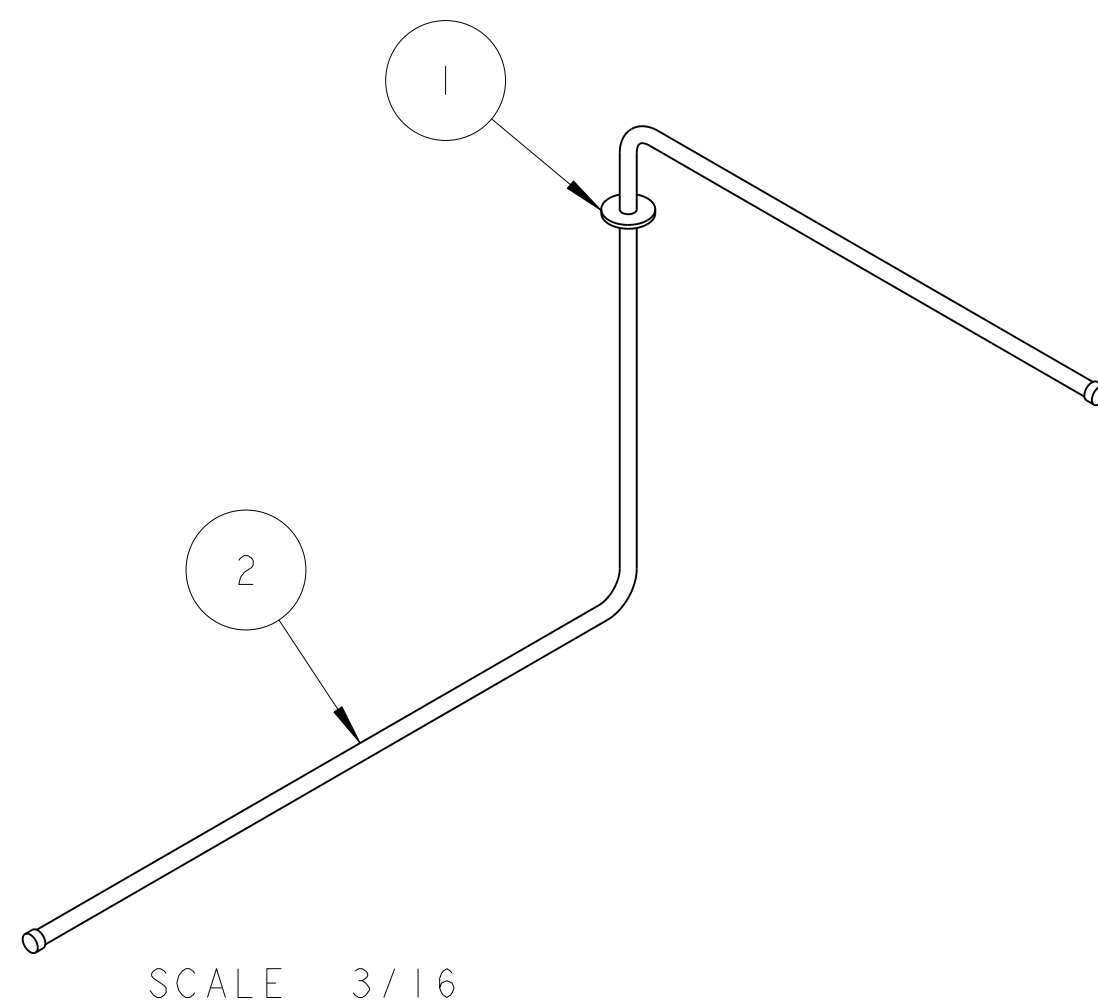

TOLERANCES		UNLESS OTHERWISE SPECIFIED		SHOP ORDERS		SER. NO.		ERNEST ORLANDO LAWRENCE				
X.X ± 0.1	FRAC. ± 1/64	ACCT. NO.	NO. REQD.	NO.	DATE ISSD.	BERKELEY NATIONAL LABORATORY						
X.XX ± 0.03	Angles ± 1.00°	DEL. TO		IDENT. TAG	DATE REQD.	UNIVERSITY OF CALIFORNIA - BERKELEY						
X.XXX ± 0.010	FINISH 125 \sqrt{Ra}	SURFACE TREATMT		PROJECT NUMBER		LHC IR FEEDBOX						
DO NOT SCALE PRINT		THREADS ARE CLASS 2		PROJECT NAME		CRYOGENICS						
CHAMFER ENDS OF ALL SCREW TRENDS 30°		CUT ROUND, 1.5 THREAD RELIEF ON MACHINED THREADS		PROJECT NUMBER		PIPE, CYI						
BREAK EDGES .016 MAX. ON MACHINED WORK		REMOVE BURRS, WELD SPLATTER & LOOSE SCALE		PROJECT NAME		MICROFILMED: DWG. TYPE SHOWN ON SCALE: 1/4 DO NOT SCALE PRINTS						
IN ACCORDANCE WITH ANSI Y14.5M & B46.1		INITIAL RELEASE		DATE 16-Apr-02		SHEET 1 OF 1						
REV	DWG	CHK	ZONE	DATE	BY	DATE	PATENT CLEAR:	DESIGN ACCT. NO.	CATEGORY CODE	DWG. NO.	SIZE	REV.
A	ARH	SPV		11-01-02	Jan Zbasnik/S.Virostek	01-Nov-02	Z5LCE2	LH2003	2515534	A		

8

7

6

5

4

3

2

1