

Officially Released to the LBNL Document Control Center
Released: July 26th, 2004 DCC Auth Key: 8JPUUYF15H

D

C


B

D

C

B

A

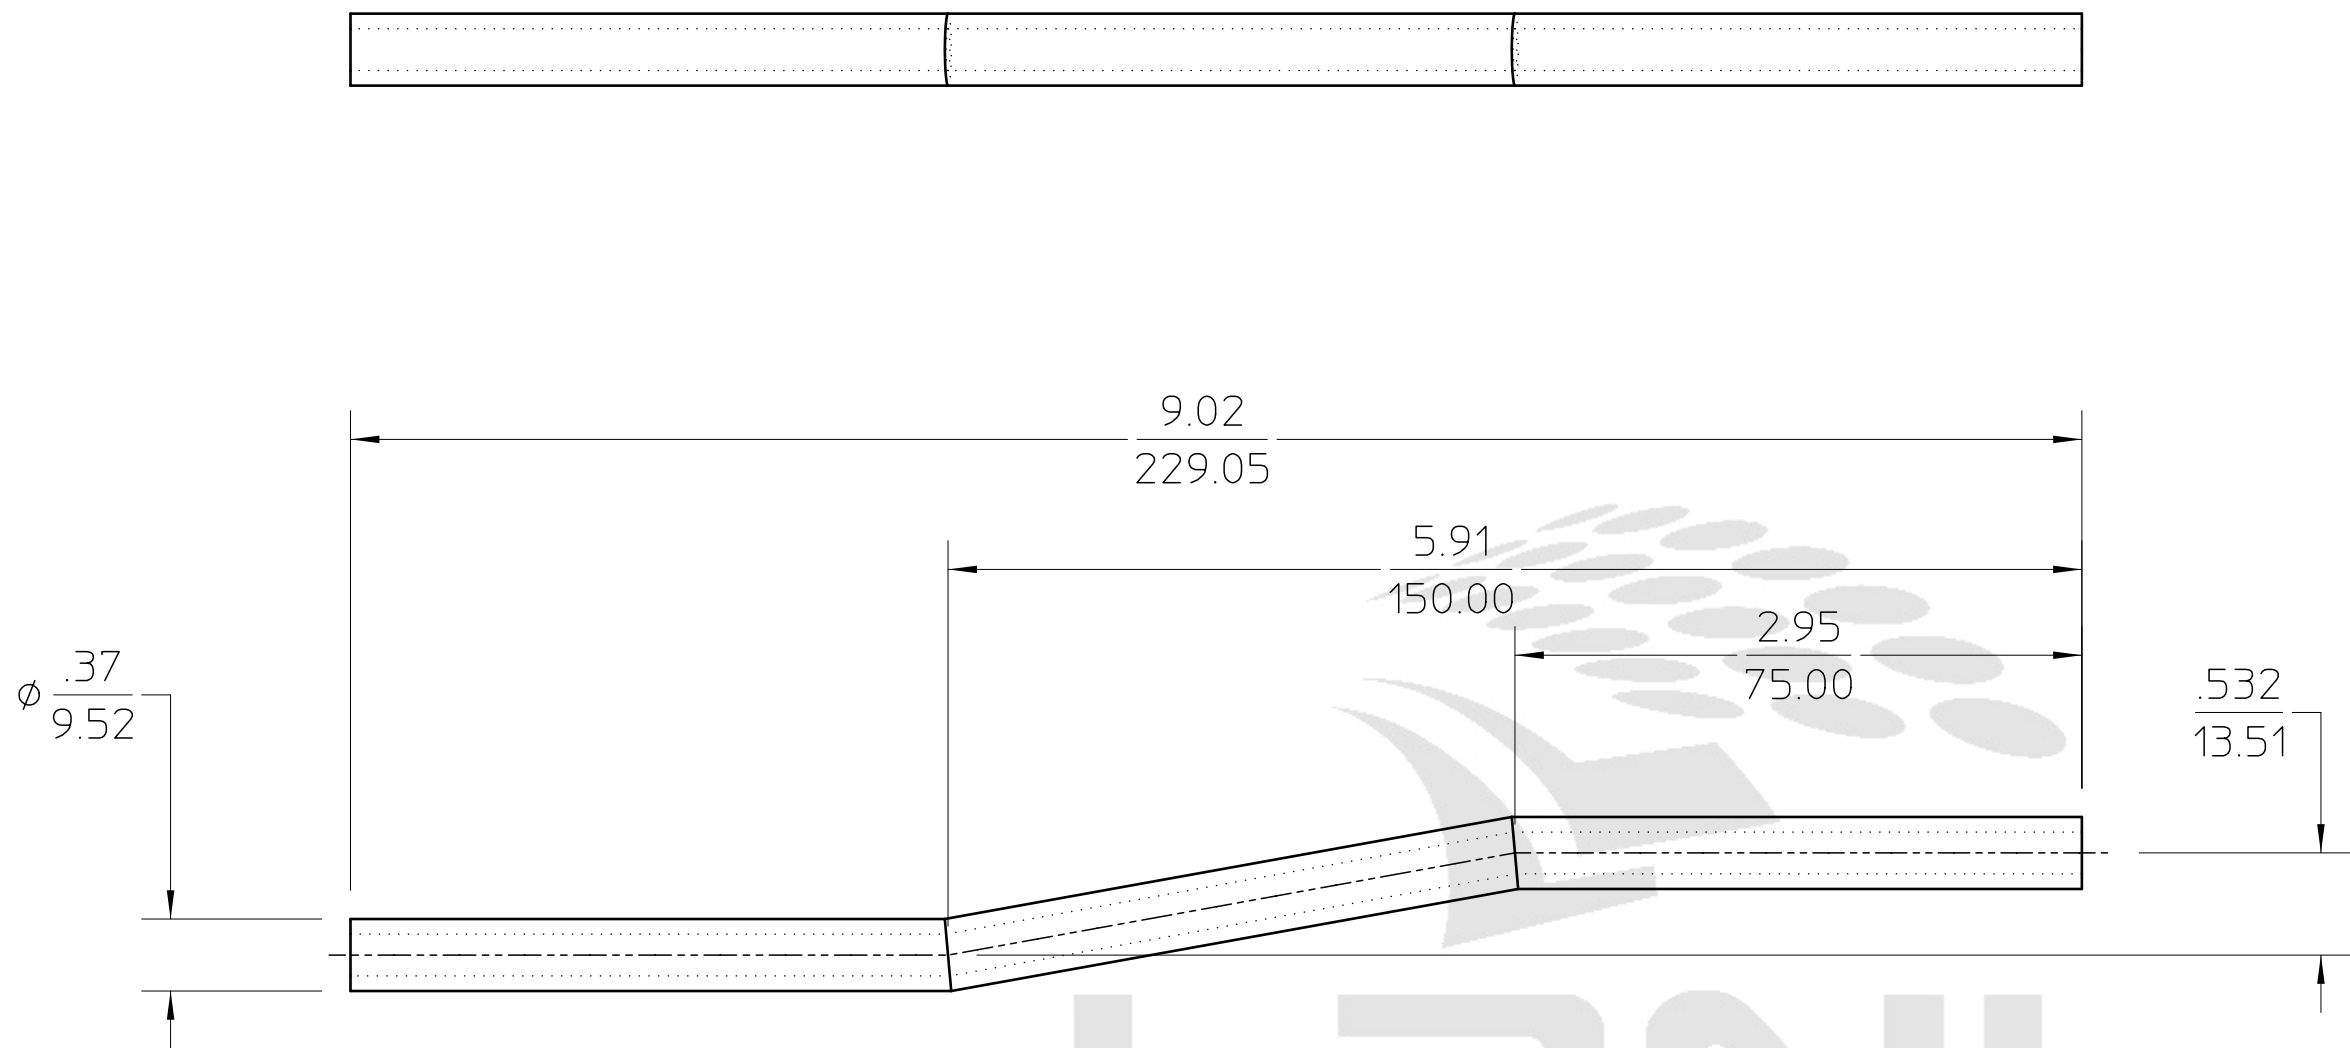

- NOTES, UNLESS OTHERWISE SPECIFIED:
- 1. THIS IS A ULTRA HIGH VACUUM COMPONENT AND REQUIRES SPECIAL ATTENTION TO AVOID CONTAMINATION. REFER TO LBNL ENGINEERING SPECIFICATION #M20013. HIGH VACUUM USE CLEANING.
 - 2. TOLERANCES SHOWN IN TITLE BLOCK ARE IN INCHES.

(UNIQUE ID NO.:AL-0008-9562)

					MAT 2: ,		NOTES:	
					MAT 1: TUBE, .375 DIA OD X .080 WALL, SST TYPE 304		NOTES:	
					PROJECT NAME: PROJECT NUMBER:		ERNEST ORLANDO LAWRENCE BERKELEY NATIONAL LABORATORY UNIVERSITY OF CALIFORNIA	
							ALS - INSERTION DEVICE BEAMLINES	
							BL 6.0 FRONT END	
							LH ABSORBER TUBE	
					DO NOT SCALE PRINT SCALE: 1 : 1		CATEGORY CODE: AL 4 160	
					THIRD ANGLE PROJECTION		SHEET 1 OF 1 SIZE: C DWG NO: 26B584 REV A	
					REF: ASME Y14.5M-1994, THREADS ARE CLASS 2 BREAK EDGES .016 MAX. ON MACHINED WORK REMOVE BURRS, WELD SPLATTER & LOOSE SCALE			
UNLESS OTHERWISE SPECIFIED								
TOLERANCES					.X ± .03 .XX ± .02 .XXX ± .010			
					FRACTIONS: ± ---			
					ANGLES: ± 1°			
					MACH. SURFS.: 63 ✓ OR BETTER			
REV					AUTHOR		APPROVER	
DATE					CHANGE		DESCRIPTION	