

D

C

B

D

C

B




A

4

3

2

1

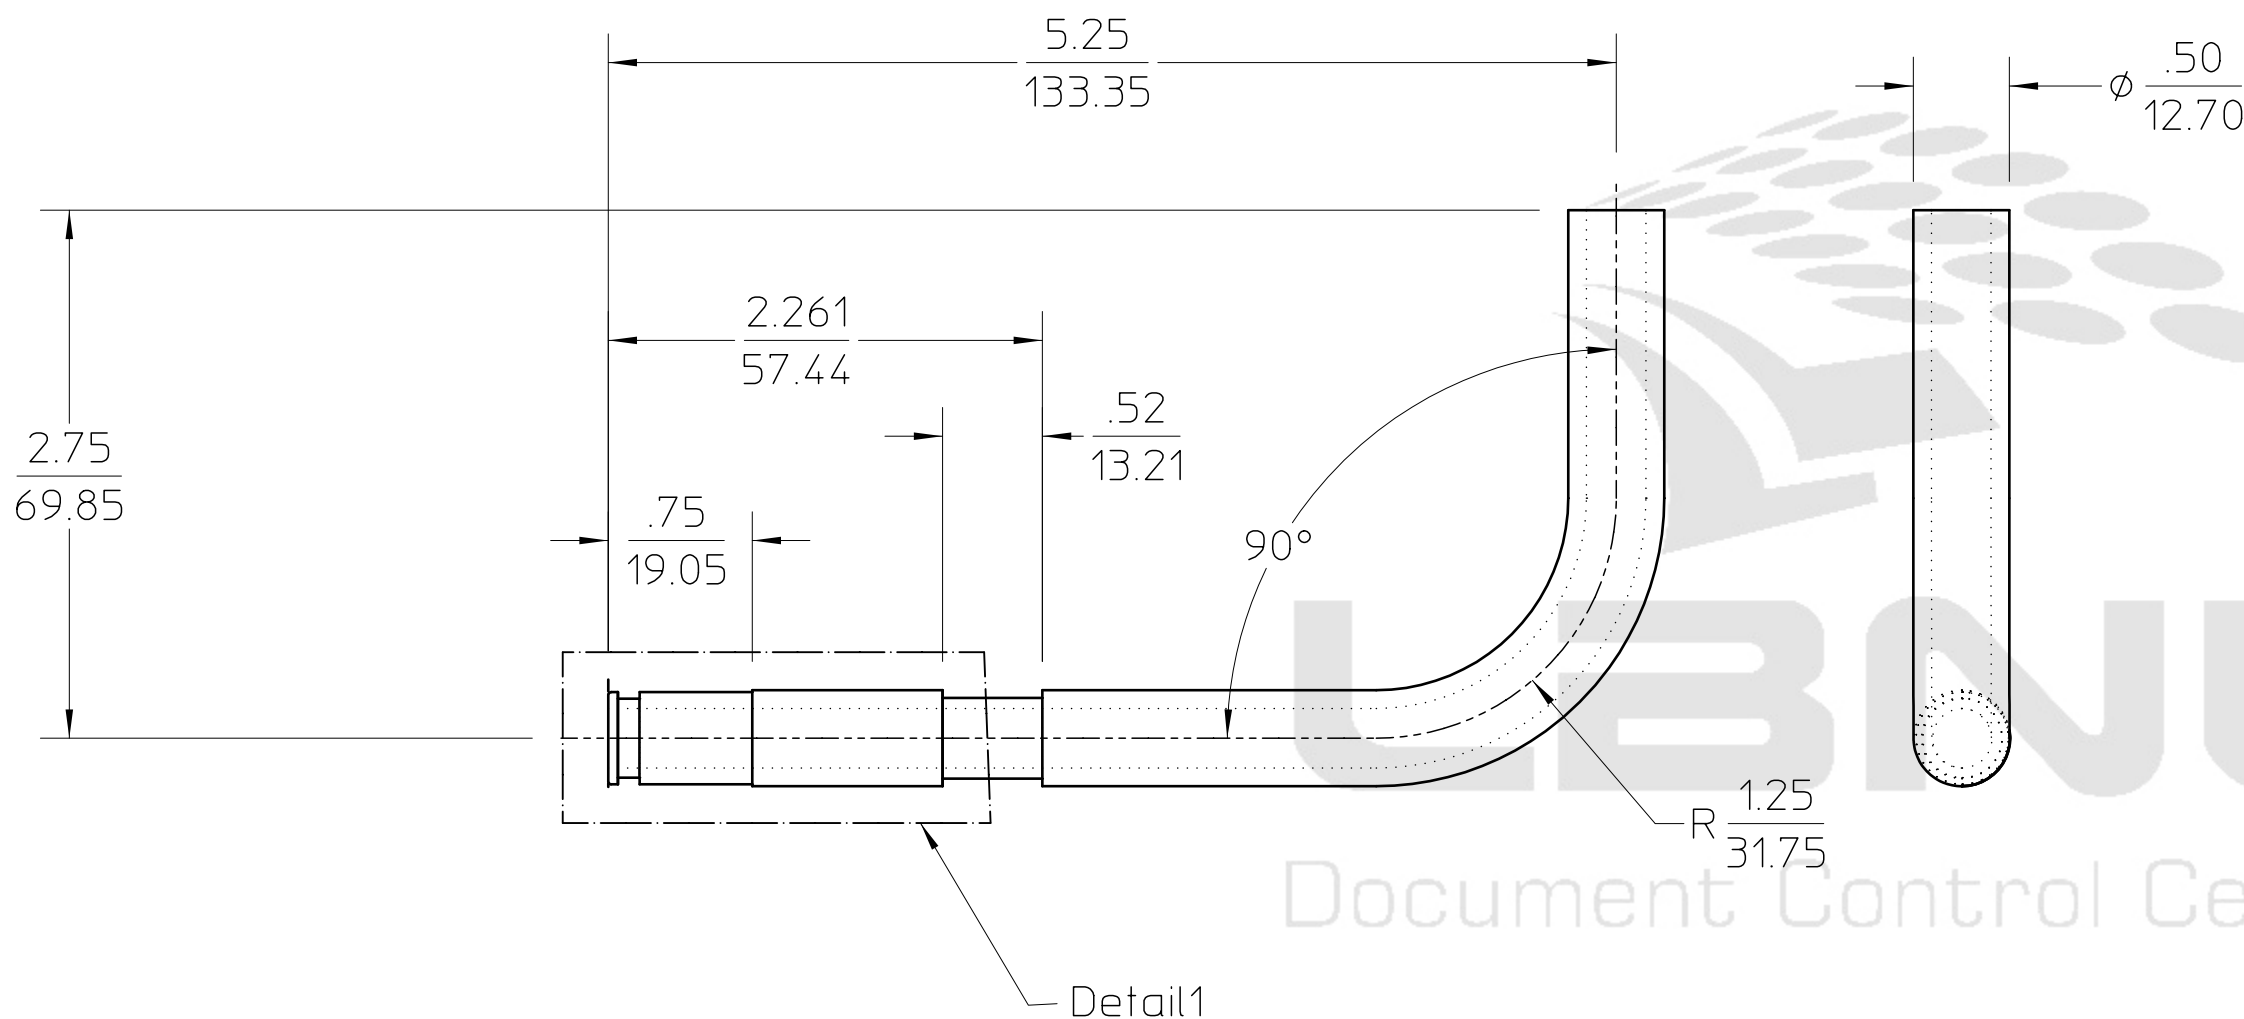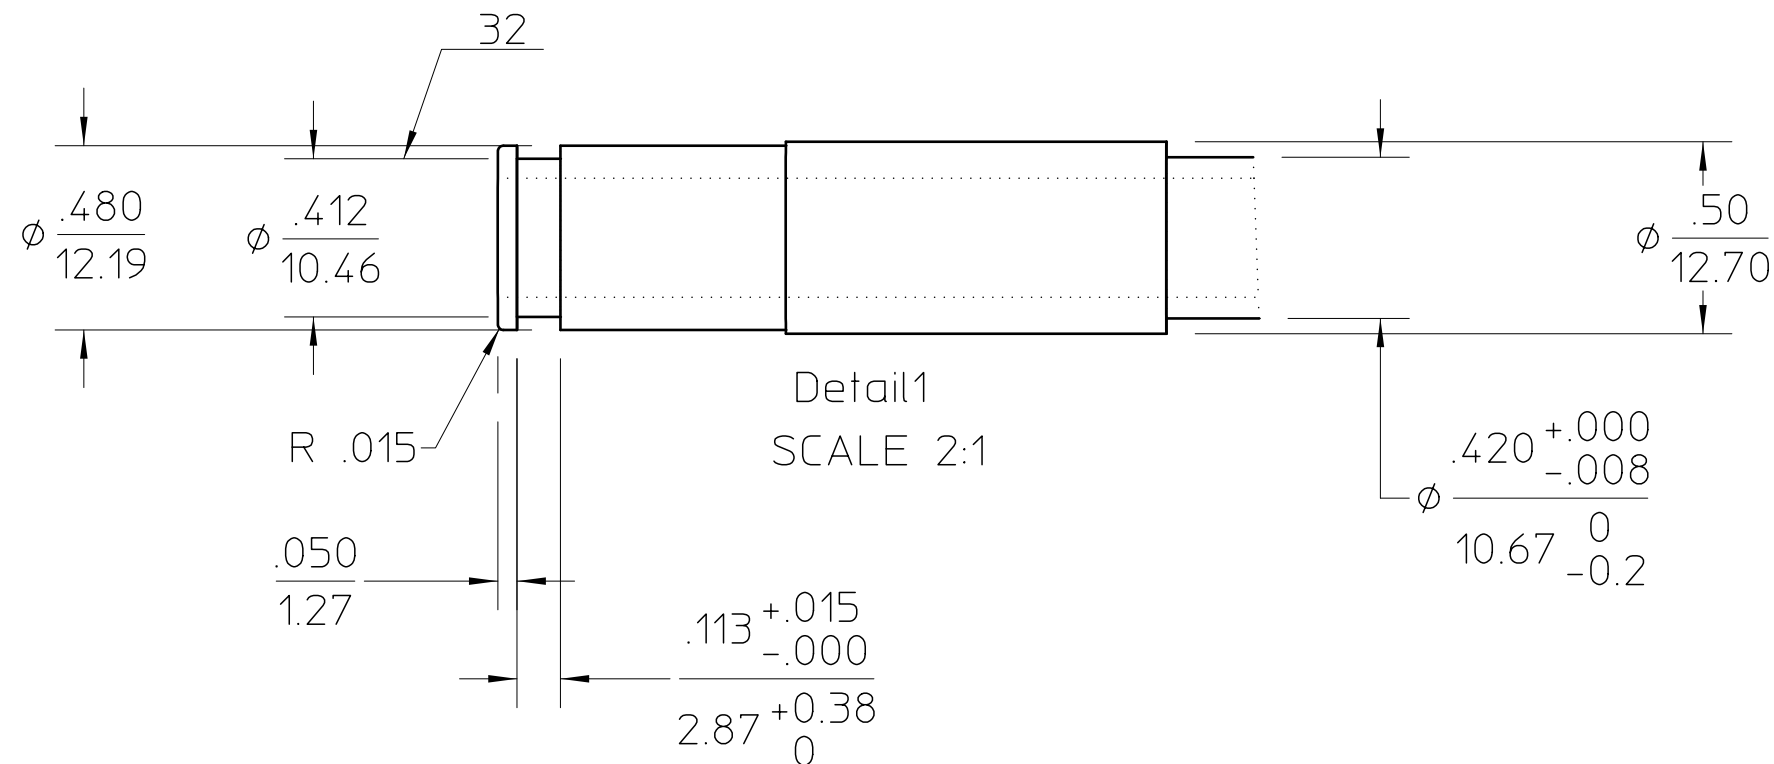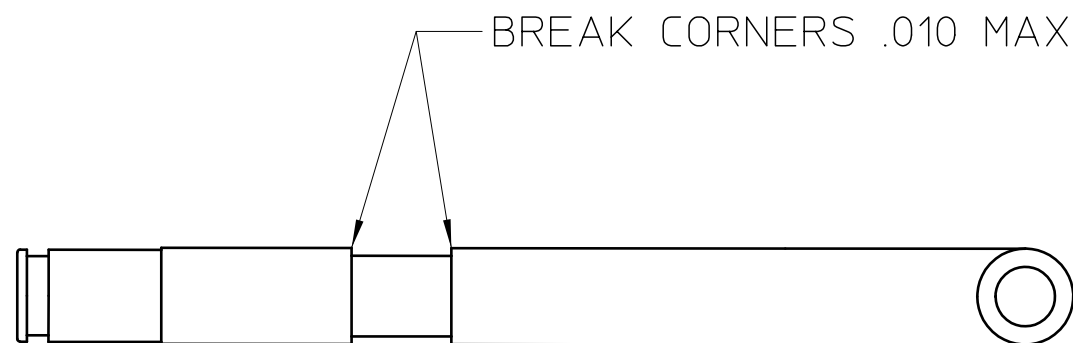

NOTES, UNLESS OTHERWISE SPECIFIED:

1. THIS IS A ULTRA HIGH VACUUM COMPONENT AND REQUIRES SPECIAL ATTENTION TO AVOID CONTAMINATION. REFER TO LBNL ENGINEERING SPECIFICATION #M20013. HIGH VACUUM USE CLEANING.
2. TOLERANCES SHOWN IN TITLE BLOCK ARE IN INCHES.

(UNIQUE ID NO.:AL-0008-9571)

SPECIFICATION #120015: HIGH VACUUM CHAMBER CLEANING					MAT 2: ,		NOTES:	
2. TOLERANCES SHOWN IN TITLE BLOCK ARE IN INCHES.					MAT 1: TUBING,304 SST,1/2"OD X .095 WALL.		NOTES:	
					UNLESS OTHERWISE SPECIFIED		PROJECT NAME: PROJECT NUMBER: ERNEST ORLANDO LAWRENCE BERKELEY NATIONAL LABORATORY UNIVERSITY OF CALIFORNIA ALS - INSERTION DEVICE BEAMLINES BL 6.0 FRONT END WATER TUBE SHEET 1 OF 1 SIZE: C DWG NO: 26B590 REV A	
					TOLERANCES			
					.X±.03 .XX±.02 .XXX±.010			
					FRACTIONS: * ---			
					ANGLES: ± 1°			
					MACH. SURFS.: 63✓ OR BETTER			
					REF:ASME Y14.5M-1994, THREADS ARE CLASS 2		DO NOT SCALE PRINT	
					BREAK EDGES .016 MAX. ON MACHINED WORK		SCALE: 1 : 1	
					REMOVE BURRS, WELD SPLATTER & LOOSE SCALE		CATEGORY CODE: AL 4160	
							THIRD ANGLE PROJECTION	
A	rawlins	plate	07-26-20	INITIAL REVISION				
REV	AUTHOR	APPROVER	DATE	CHANGE DESCRIPTION				

3

2