

Officially Released to the LBNL Document Control Center
Released: January 19th, 2005 DCC Auth Key: QC461WNZBX

D

C




B

D

C

B

A

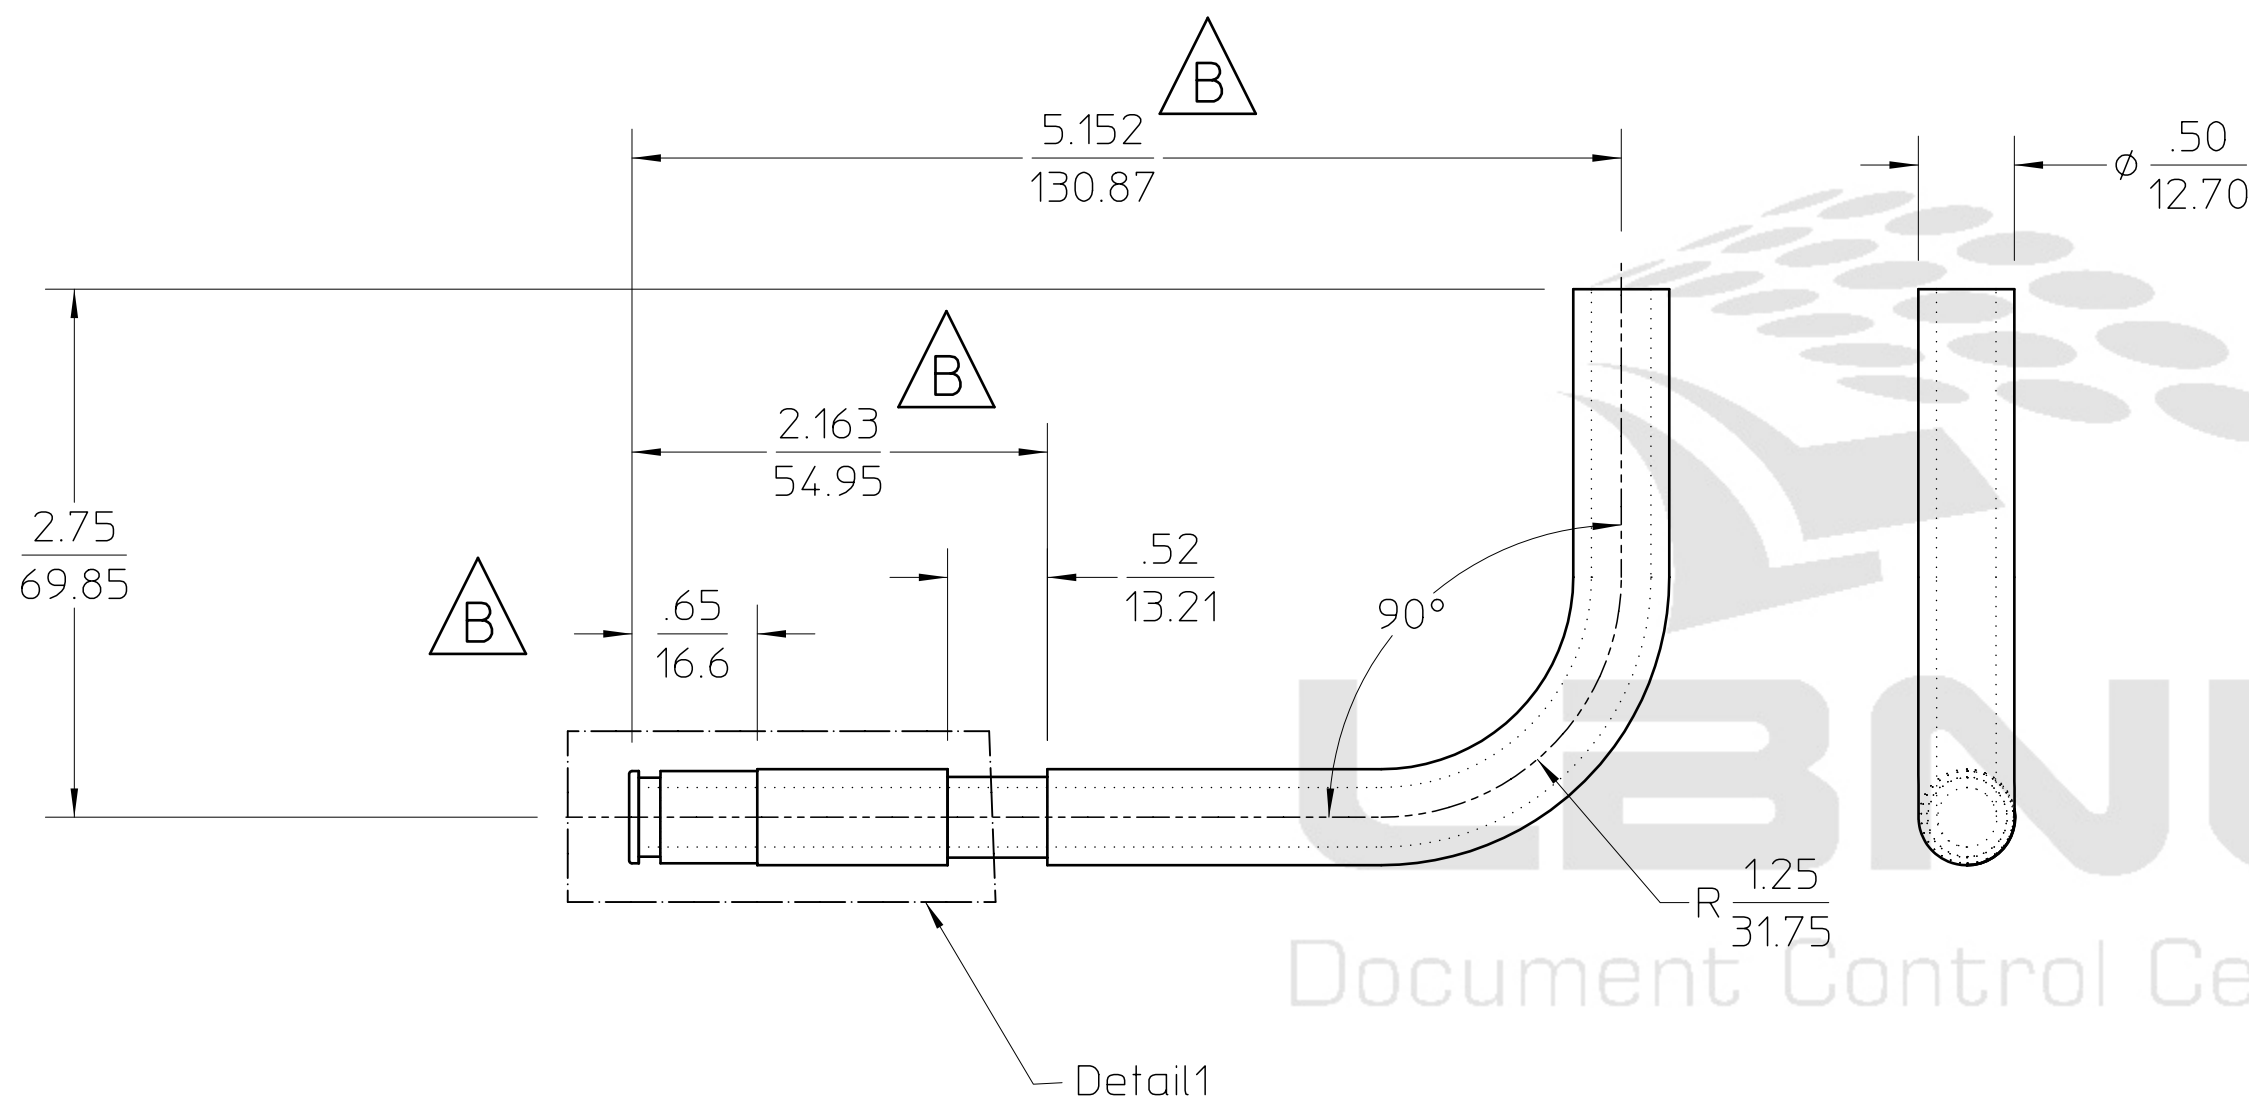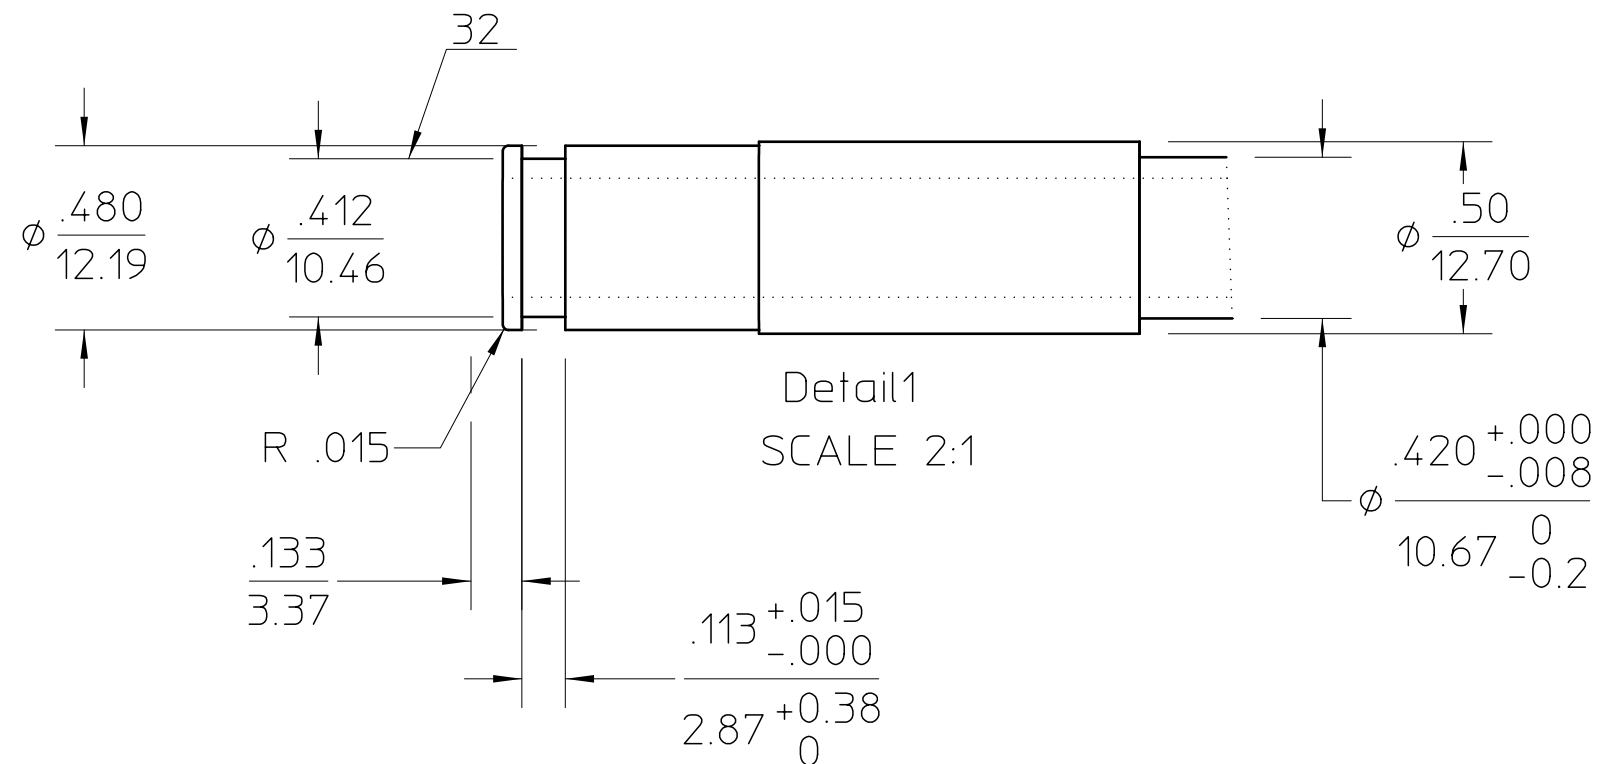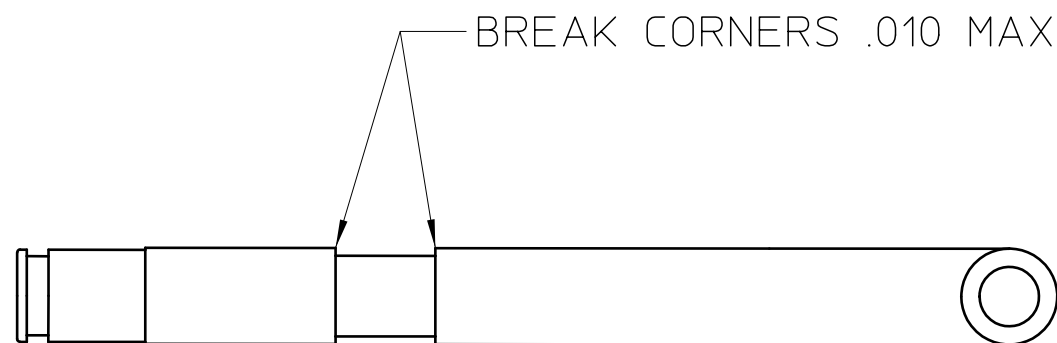

NOTES,UNLESS OTHERWISE SPECIFIED:

1. THIS IS A ULTRA HIGH VACUUM COMPONENT AND REQUIRES SPECIAL ATTENTION TO AVOID CONTAMINATION. REFER TO LBNL ENGINEERING SPECIFICATION #M20013. HIGH VACUUM USE CLEANING.
2. TOLERANCES SHOWN IN TITLE BLOCK ARE IN INCHES.

(UNIQUE ID NO.:AL-0008-9571)

					MAT 2: ,		NOTES:	
					MAT 1: TUBING,304 SST,1/2"OD X .095 WALL.		NOTES:	
					PROJECT NAME: PROJECT NUMBER:		ERNEST ORLANDO LAWRENCE BERKELEY NATIONAL LABORATORY UNIVERSITY OF CALIFORNIA ALS - INSERTION DEVICE BEAMLINES BL 6.0 FRONT END WATER TUBE	
B	cummings	plate	01-19-05	OVERALL LENGTH CHANGED	REF:ASME Y14.5M-1994, THREADS ARE CLASS 2		DO NOT SCALE PRINT	
A	rawlins	plate	07-26-04	INITIAL REVISION	BREAK EDGES .016 MAX. ON MACHINED WORK		CATEGORY CODE: AL 4 160	
REV	AUTHOR	APPROVER	DATE	CHANGE DESCRIPTION	REMOVE BURRS, WELD SPLATTER & LOOSE SCALE		THIRD ANGLE PROJECTION	
							SHEET 1 OF 1	
							SIZE: C	
							DWG NO: 26B590	
							REV B	